

# **QT-Brightek Chip LED Series**

## **SMD 0805 Green LED**

**Part No.: QBLP631-IG-2897**

**2897: High Brightness Version**

Product: QBLP631-IG-2897	Date: March 27, 2024	Page 1 of 9
	Version# 1.0	

---

**Table of Contents:**

Introduction .....	3
Electrical / Optical Characteristic (Ta=25 °C) .....	4
Absolute Maximum Rating .....	4
Characteristic Curves.....	5
Solder Profile & Footprint.....	6
Packing .....	7
Labeling .....	8
Ordering Information .....	8
Revision History .....	9
Disclaimer .....	9

## Introduction

### Feature:

- Water clear lens
- Package in tap and reel
- 0805 LED package
- InGaN technology
- Viewing angle: 140 deg typ.

### Description:

These ultra bright 0805 LEDs have a height profile of 0.8mm. Combination of high brightness output and small footprint, these LEDs are ideal for keypad backlighting and status indication.

### Application:


- Status indication
- Back lighting application

### Certification & Compliance:

- ISO9001
- RoHS Compliant



## Dimension:

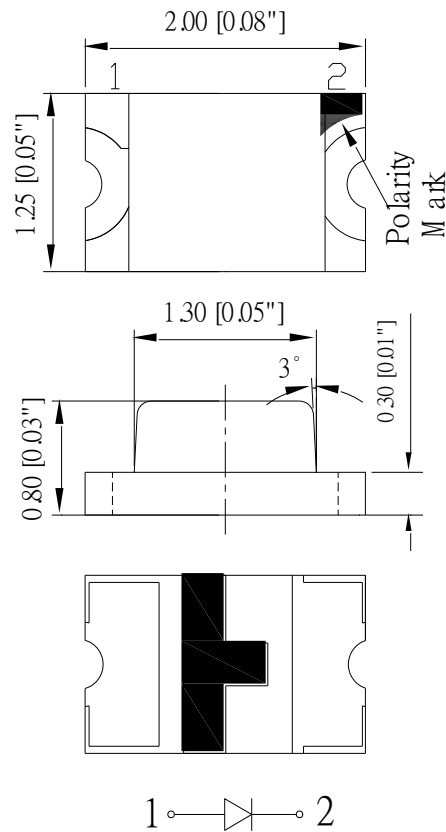

Units: mm / tolerance = +/-0.1mm

### Electrical / Optical Characteristic (Ta=25 °C)

Product	Color	I <sub>F</sub> (mA)	V <sub>F</sub> (V)		λ <sub>D</sub> (nm)			λ <sub>P</sub> (nm)	I <sub>V</sub> (mcd)	
			Typ.	Max.	Min.	Typ.	Max.	Typ.	Min.	Typ.
QBLP631-IG-2897	Green	20	2.7	3.4	520	525	530	520	630	1200

### Absolute Maximum Rating

Material	P <sub>d</sub> (mW)	I <sub>F</sub> (mA)	I <sub>FP</sub> (mA)*	V <sub>R</sub> (V)	T <sub>OP</sub> (°C)	T <sub>ST</sub> (°C)	T <sub>SOL</sub> (°C)**
InGaN	102	30	125	5	-40 ~ +80	-40 ~ +85	260

\*Duty 1/8 @ 1KHz

\*\*IR Reflow for no more than 10 sec @ 260 °C

### Forward Voltage V<sub>F</sub> @ I<sub>F</sub>=20mA

Bin	Min.	Max.	Unit
e	2.5	2.8	V
f	2.8	3.1	
g	3.1	3.4	




### Luminous Intensity I<sub>V</sub> @ I<sub>F</sub>=20mA

Bin	Min.	Max.	Unit
R	630	800	mcd
S	800	1000	
T	1000	1250	
U	1250	1600	
V	1600	2000	

### Dominant Wavelength λ<sub>D</sub> @ I<sub>F</sub>=20mA


Bin	Min.	Max.	Unit
U	520	522.5	nm
V	522.5	525	
W	525	527.5	
X	527.5	530	

**Characteristic Curves**

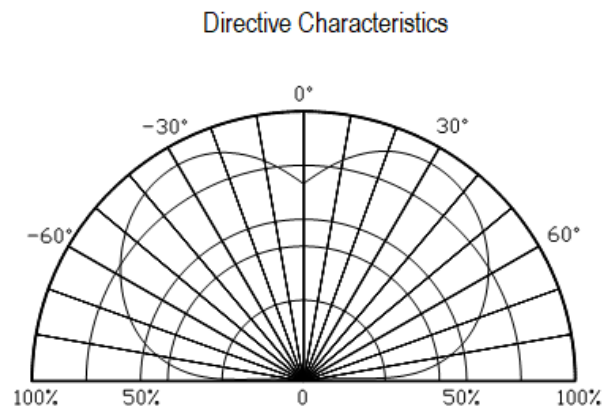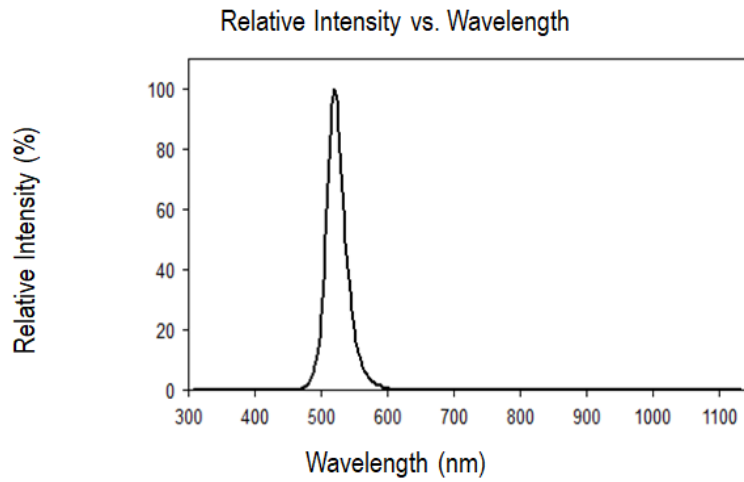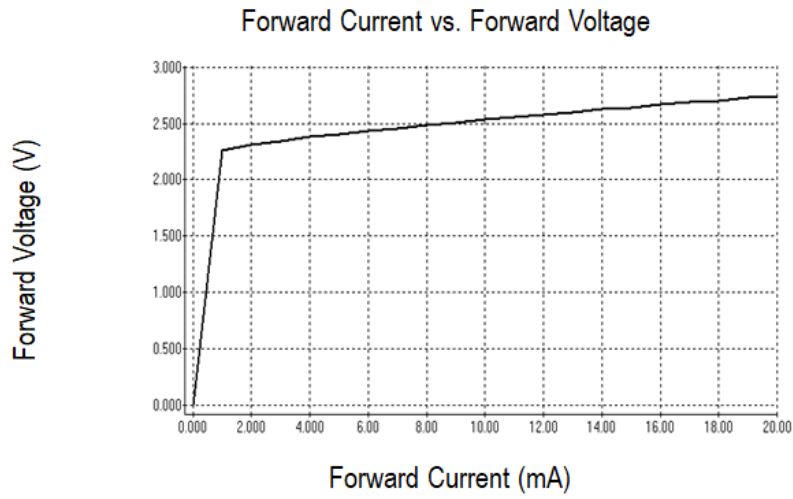


**Solder Profile & Footprint**

-The recommended reflow soldering profile is as follows (temperatures indicated are as measured on the surface of the LED resin):

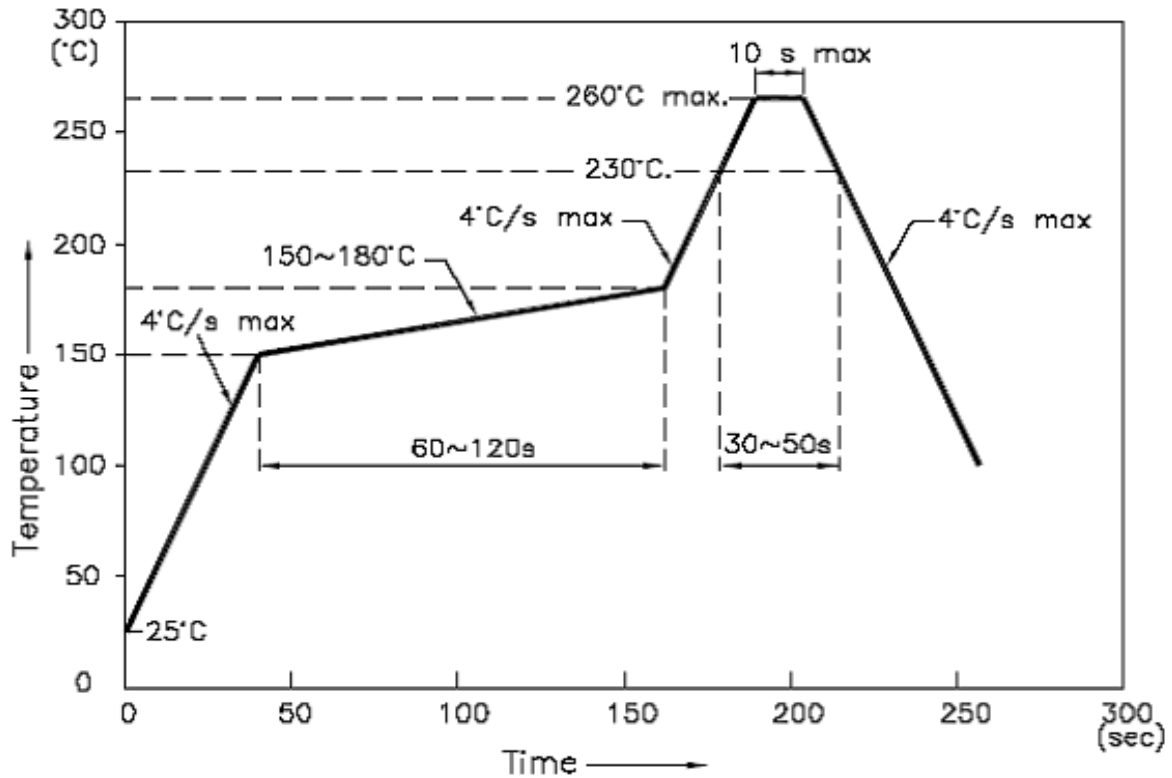


**Recommended Pad Layout**

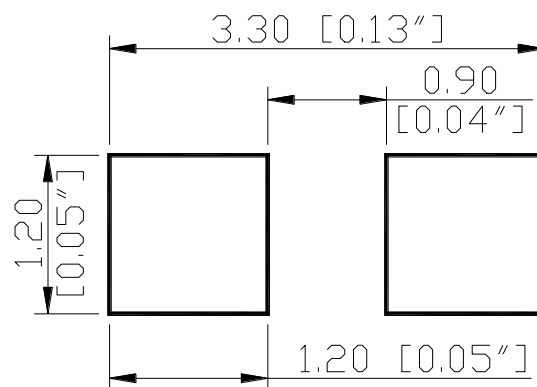

Units: mm


## Packing

### Reel Dimension:

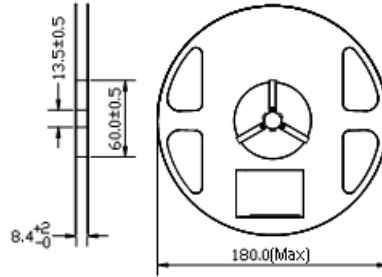


Unit: mm

### Tape Dimension:

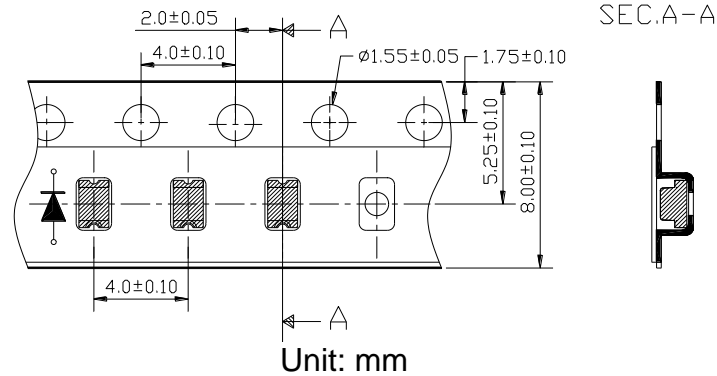


Unit: mm

### Arrangement of Tape:

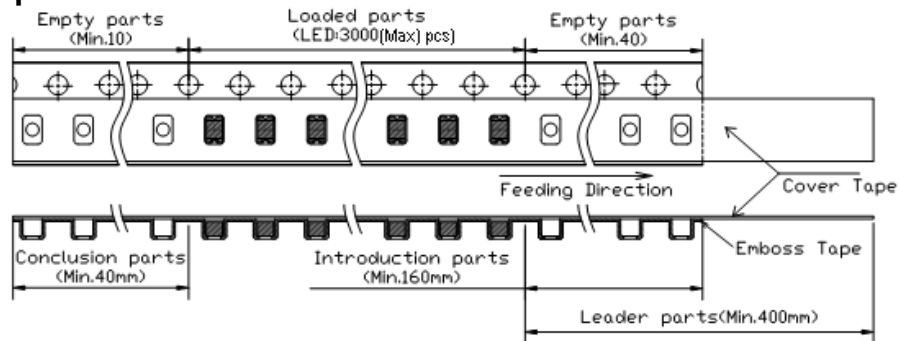

### Packaging Specification:

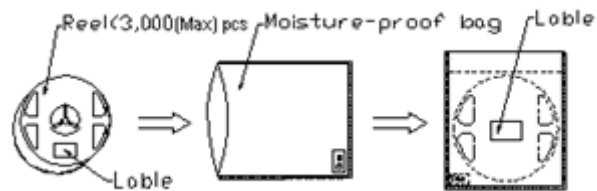

**Labeling**

Part No: \_\_\_\_\_

Customer P/N: \_\_\_\_\_

Item: \_\_\_\_\_

Q'ty: \_\_\_\_\_

Vf: \_\_\_\_\_

Iv: \_\_\_\_\_

VI: \_\_\_\_\_

Date: \_\_\_\_\_

**Made in China****Ordering Information**

Orderable Part #	Spec Range	Quantity per reel
QBLP631-IG-2897	Iv=1200mcd typ. / λ <sub>D</sub> = 520nm to 530nm @ 20mA	3000 units

Product: QBLP631-IG-2897	Date: March 27, 2024	Page 8 of 9
	Version# 1.0	



---

## Revision History

Description:	Revision #	Revision Date
New Release of QBLP631-IG-2897	V1.0	03/27/2024

---

## Disclaimer

QT-BRIGHTTEK reserves the right to make changes without further notice to any products herein to improve reliability, function or design. QT-BRIGHTTEK does not assume any liability arising out of the application or use of any product or circuit described herein; neither does it convey any license under its patent rights, nor the rights of others.

## Life Support Policy

QT-BRIGHTTEK's products are not authorized for use as critical components in life support devices or systems without the express written approval of QT-BRIGHTTEK. As used herein:

1. Life support devices or systems are devices or systems which, (a) are intended for surgical implant into the body, or (b) support or sustain life, and (c) whose failure to perform when properly used in accordance with instructions for use provided in the labeling, can be reasonably expected to result in a significant injury of the user.
2. A critical component in any component of a life support device or system whose failure to perform can be reasonably expected to cause the failure of the life support device or system, or to affect its safety or effectiveness.